



THOR 50th Left Ankle Eversion Test

Test Parameter	min	Max	Unit	Result	Pass/Fail
Temperature	20.6	22.2	°C	21.0	Pass
Humidity	10	70	%	40.0	Pass
Impact Velocity	1.95	2.05	m/s	2.00	Pass
Peak Lower Tibia Fz	-629	-514	N	-587.72	Pass
Peak Ankle Resistive Moment	38.7	47.3	Nm	44.95	Pass
Peak Ankle X-axis Rotation	26.6	32.5	deg	28.00	Pass

Lower Tibia Z-axis Force

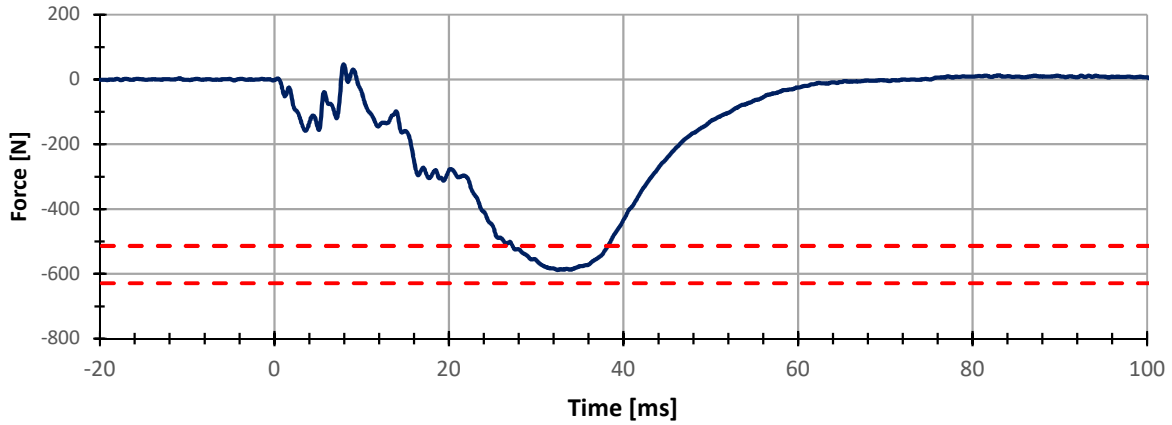

Ankle Resistive Moment

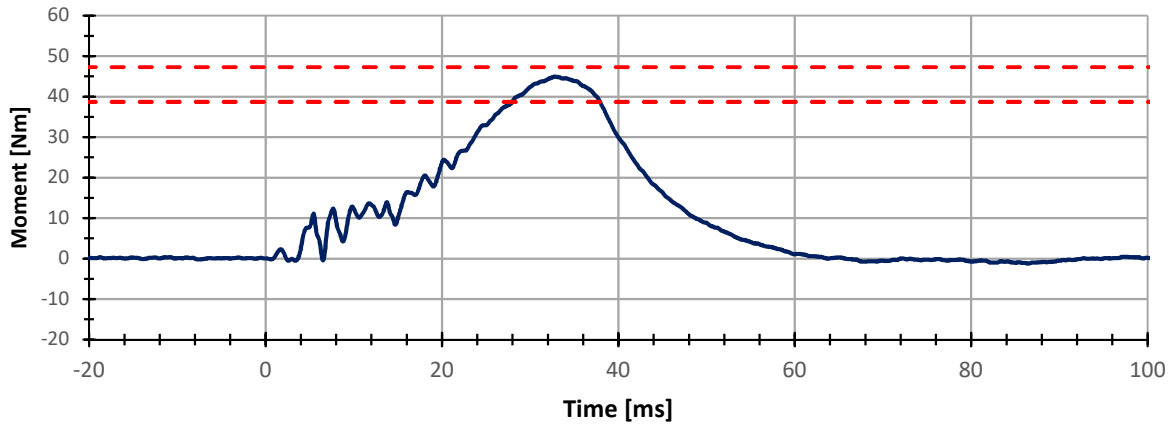

Ankle X-axis Rotation

